




MXT

100g x 0.01g / 500g x 0.1g

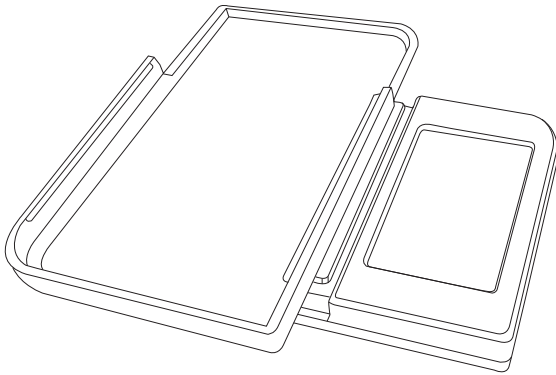

USER MANUAL

MXT

100g x 0.01g / 500g x 0.1g



Thank you for purchasing the My Weigh® MXT digital pocket scale. Please read all operating instructions carefully before use. This electronic scale is a precision instrument. With normal care and proper treatment, it will provide years of reliable service. For more information please visit www.myweigh.com.

BATTERIES

Battery installation

- a) Press and lift open the battery cover located at the bottom of the unit.
- b) Insert the batteries and make sure the polarity is correct.
- c) Close the battery cover until it clicks shut.

Note : If the battery symbol appears in the display, it means low battery power. It is time to replace the batteries.

OPERATION INSTRUCTIONS

Weighing Procedures

1. Press [ON/OFF] to turn on or off the scale.
2. Press [MODE] to select a weighing unit g, oz, dwt, ozt.
3. Start weighing.

Tare

Tare can be used for eliminating the weight value of an empty container. Place an empty container on the scale and press [TARE]. After 3 seconds place the items to be weighed in the container. NOTE: When all weight is removed from the weighing tray, the tared value of a container will be displayed as a negative number. Press [TARE] again to return the scale to zero.

CALIBRATION

Calibration may be required when the scale is first set up for use, or if the scale is moved to a different altitude or new location. This is necessary because the weight of a mass in one location is not necessarily the same in another location. Also, with time and use, mechanical deviations can occur.

To Calibrate the MXT 100: *you must have an accurate 100g weight in order to calibrate.*

1. Place the scale on a flat, very stable surface and turn on the scale.
2. Press and hold the [MODE] key for 3 seconds, the display will show "CAL" and then the correct calibration weight.
3. Gently place the 100g weight on the tray and wait for 3 seconds.
4. Press the [ON/OFF] key. The display will show "PASS", and then will return to normal weighing mode. Calibration is now complete.

To Calibrate the MXT 500: *you must have an accurate 300g weight in order to calibrate.*

1. Place the scale on a flat, very stable surface and turn on the scale.
2. Press and hold the [MODE] key for 3 seconds, the display will show "CAL" and then the correct calibration weight.
3. Gently place the 100g weight on the tray and wait for 3 seconds.
4. Press the [ON/OFF] key. The display will show "PASS", and then will return to normal weighing mode. Calibration is now complete.

FEATURES

Power Up Segment Test

When first turning the unit on, the scale will run a quick diagnostic and it will display a countdown . This display will remain for a few seconds and then reset to zero.

Overload indicator

When the display shows “O-LD”, this indicates an overload. Remove excessive load immediately. Remember: you can permanently damage the scale and void your warranty by overloading it!

Negative Value

Any tared value will be displayed as a negative number once all weight is removed, press [TARE] to re-zero the scale.

Auto off

An auto off feature is provided to conserve battery power. The unit will automatically turn off after 3 minutes of inactivity.

Expansion Tray/Cover

The protective cover of the MXT is designed to also be used as a platform expansion tray.

SPECIFICATIONS		
Model	MXT 100	MXT 500
Capacity	100g x 0.01g	500g x 0.1g
Units	g, oz, ct, gn	g, oz, dwt, ozt
Auto-OFF	3 mins	
Scale dimension	89mm x 53mm x 12mm / 3.5" x 2.3" x 0.6"	
Tray dimension	53mm x 46mm / 2.3" x 1.8"	
Scale weight	65g / 2.3oz	
Operating temperature	Optimum 10-40°C (50-104°F)	
Power Source	2 x CR2032 Batteries	
Tare range	Up to scale's maximum capacity	



www.myweigh.com